

Packages securely and reliably – The new Hygopac Plus

Sterile goods packaging for state-of-the-art medical practice – meeting all legal requirements



COMPRESSED AIR
SUCTION
IMAGING
DENTAL CARE
HYGIENE
▪ INSTRUMENTS



The new Hygopac Plus – Quick sterile-goods packaging, secure and verifiable

Instrument packaging has never been so easy and reliable.

You can rest assured that each individual package meets the requirements of standard DIN EN ISO 11607-2 and the guidelines of the German Association for Sterile Services (DGSV).



Overview of Hygopac Plus

- Intelligent validation concept
- Process control
- Integrated process monitoring
- Data storage with SD card or network
- High sealing speed
- Requires minimum space
- Intuitive operation
- Elegant, functional design
- Compliant with safety standards
- Sealing with a built-in system

Sterile packaging as a bag or from the roll. Pack it with Hygofol


Save time with fast, standard-compliant packaging and reduce costs with roll products – now with practical ruler to cut to the optimal length. Can be used with or without the flexible Hygofol Station.



A new validation experience. According to the applicable medical device for operators regulation, the preparation of goods with a medical device must be performed using a suitable validated process. This is no problem with the new Hygopac Plus! Sealing temperature, pressing pressure and sealing speed are verified while continuously collected, checked and saved by the device. **This means validation is 100%.**




To animation

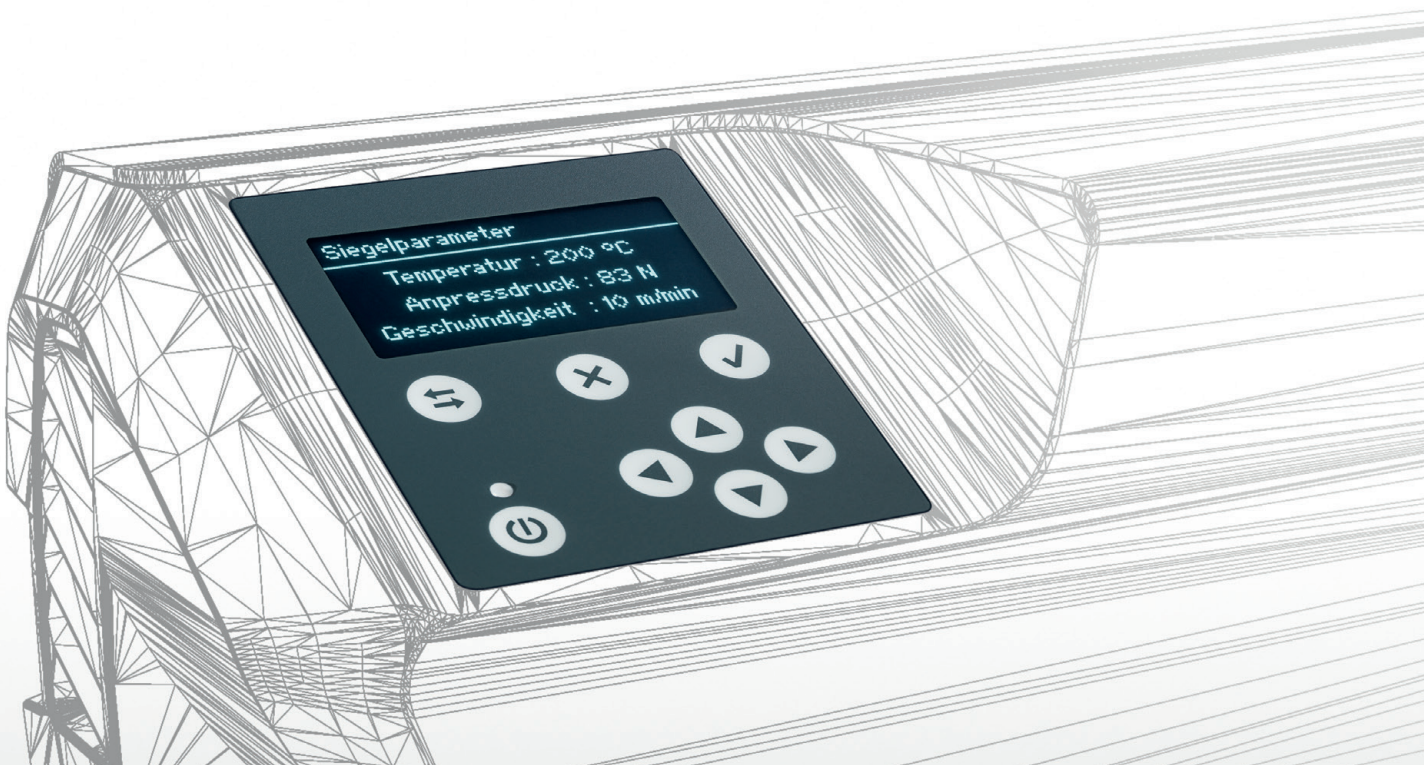


Systematic sealing: You can almost work blindfolded thanks to the accessories and packaging foil from the Hygopac Plus System. The daily seal-seam test makes it possible to check the Hygoseal's seal-seam quality at a glance and every day for added security and reassurance.



Instrument table and Hygofol Station for table mounted use

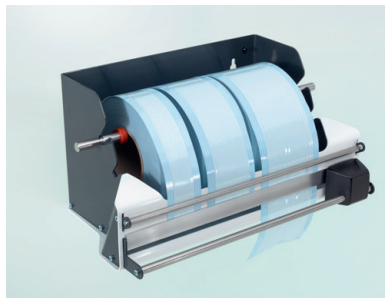

Hygofol Station wall mounted

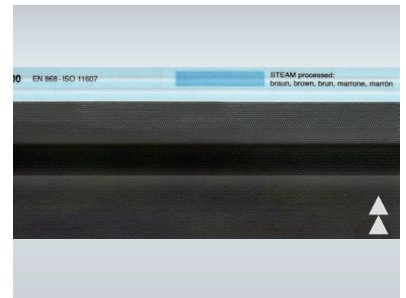

Hygoseal, daily seal-seam test

Hygopac

Sealing device for transparent sterile packaging

Hygopac Plus

Verifiable Sealing device in accordance with
DIN EN ISO 11607-2



Hygopac

Hygopac Plus

Technical data

Voltage	230 V	230 V
Electrical frequency	50 - 60 Hz	50 - 60 Hz
Power output	550 W	550 W
Heating performance	2 × 250 W	2 × 250 W
Warm-up time	approx. 3 min	approx. 3 min
Sealing temperature	to 240 °C	to 220 °C
Temperature adjustment	stepless	exact in 5 °C increments
Sealing speed	5.3 m/min	10 m/min
Seal-seam width	9 mm	12 mm
Weight	7.2 kg	7.2 kg
Dimensions (H × W × D)	160 × 435 × 135 mm	170 × 370 × 140 mm
Time saved in comparison to bar-sealing devices	●	●
Control panel with display		●
Validation		
Process control (sealing temperature, sealing speed, pressing pressure)		●
Function assessment	●	●
Manufacturer performance assessment	●	●
Storage of important parameters		●
Automatic data storage via SD card or network		●
Optional accessories		
Instrument table	●	●
Roll cutting mechanism	●	●